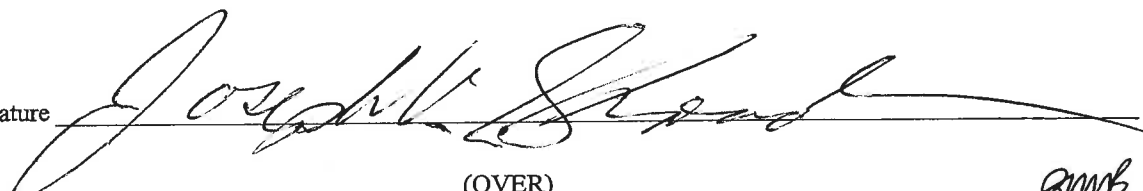


VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska


Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Supervisor/Operator Performing the Verification Procedure:		DataMaster cdm S/N	130526
Name		Joseph V. SHOEMAKER	ID# 488 Date 2-29-12
A	Agency	(SPD) Sand Point Police Dept	Phone # 907 383 3700
Instrument Location		Sand Point Police Dept SAND Point, AK	
Alco S/N		130526	Target Value .080 High Pressure 700
B	Alco Test Value Average		.077 1 st Alco .075 2 nd Alco
Signature			
		(OVER)	

(Do Not write in the area below)

I, Nita J. Bolz, after being first duly sworn, depose and state as follows:

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.

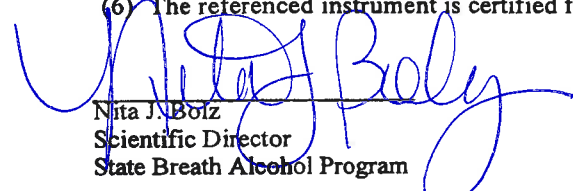

Nita J. Bolz
Scientific Director
State Breath Alcohol Program

Subscribed and sworn before me this 5 day of April 2012



Nikki Roth, Notary Public
My Commission Expires With Office

BT9 03/00



VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N

130526

(CONTINUED FROM FRONT PAGE)

C

TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130526

FEBRUARY 29, 2012

OPERATOR'S NAME:
SUPERVISOR

OPERATOR'S NUMBER: 4188

SUBJECT'S LAST NAME:

VERIFICATION OF CAL

SUBJECT'S FIRST NAME/MI :

L

O.L. #: L

DEPT/AGENCY: SDP1

CASE/REPORT: L

TEST TYPE: V

ALCO TARGET VALUE: .000

ALCO S/N: 130526-4W BMB 3/7/12

--- BREATH ANALYSIS ---

.000 ADJUSTED FOR 29.72 in

ALCO TARGET .079 17:08

BLANK TEST .000 17:09

INTERNAL STANDARD VERIFIED 17:09

ALCO TV 29.72 in .077 17:10

BLANK TEST .000 17:10

SUBJECT SAMPLE BMB 3/7/12 .000 17:11

BLANK TEST .000 17:12

ALCO TV 29.70 in .075 17:12

BLANK TEST .000 17:13

DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130526

FEBRUARY 29, 2012

TIME 17:18

--- DIAGNOSTIC CHECK ---

COMPUTER: OKAY

PROGRAM: OKAY

SOFTWARE DATE: 02/20/01

HEATERS

SAMPLE CHAMBER: 49c

BREATH TUBE: 42c

BAROMETER: 29.70 in

FLOW DETECTOR: OKAY

PUMP

HIGH SPEED: OKAY

DETECTOR: OKAY

FILTERS: OKAY

QUARTZ STANDARD: OKAY

CALIBRATION: OKAY

PRINTER TEST

!"#\$%&'()*+,-./0123456789:;<=>?@ABCDEFGHIJ
KLMNOPQRSTUVWXYZ[\]^_`abcde fghijklmno
pqrstuvwxyz{|}~"